



Magnetic Bite Fork Support Instructions

1

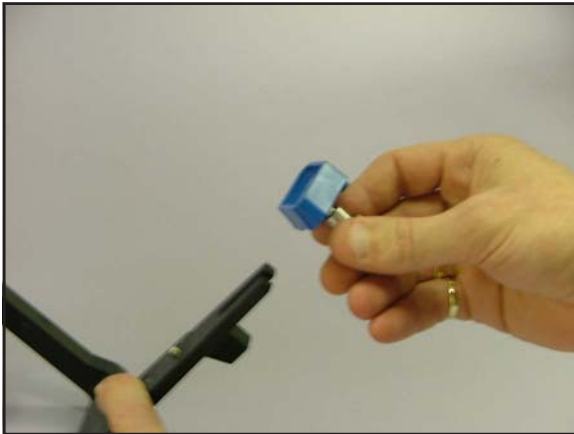


Remove plastic incisal table from articulator.

2

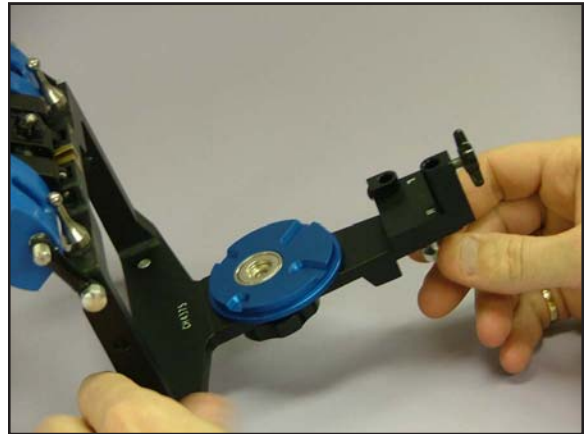


Place mounting fixture into incisal table slot and lock with thumb screw.

3

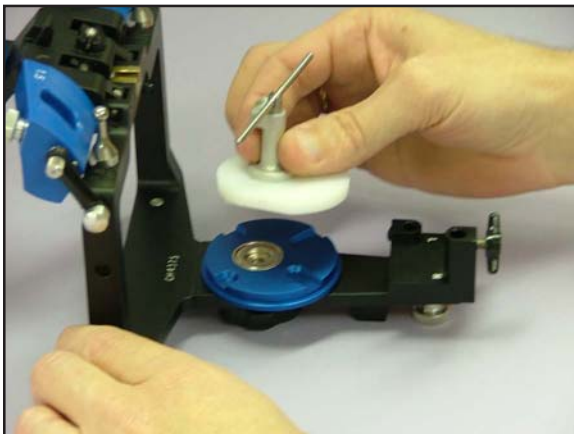


Index magnetic bite fork support to magnetic mounting plate on lower frame of articulator.

4

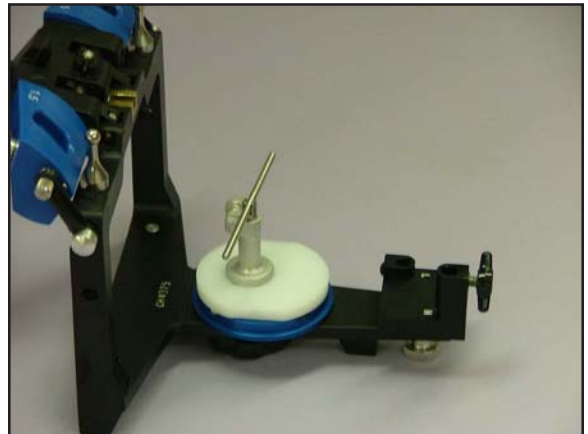

Make sure cast support rod is adjusted all the way down.

5

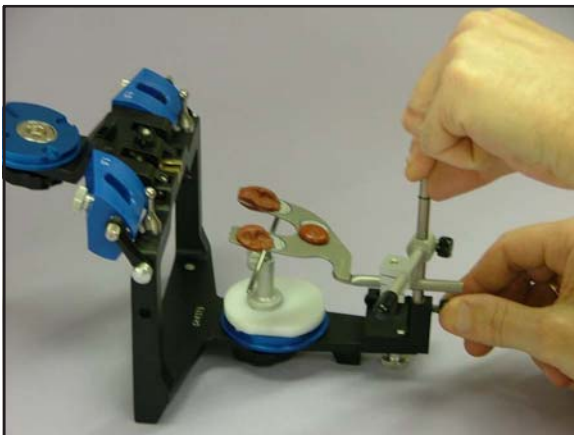

Place and lock bite fork assembly into mounting fixture.

6



Gently pull cast support rod up until it touches bite fork and lock in place with thumb screw. Mount study cast in usual manner.